

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 43
 Customer: Framtiden i våre hender
 Customers sample ID: Mc Donalds,
 French Fries pose pommes frites
 Type of sample: Matemballasje
 Sample amount (g): 2.76
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	19.4
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.62
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.64
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 43

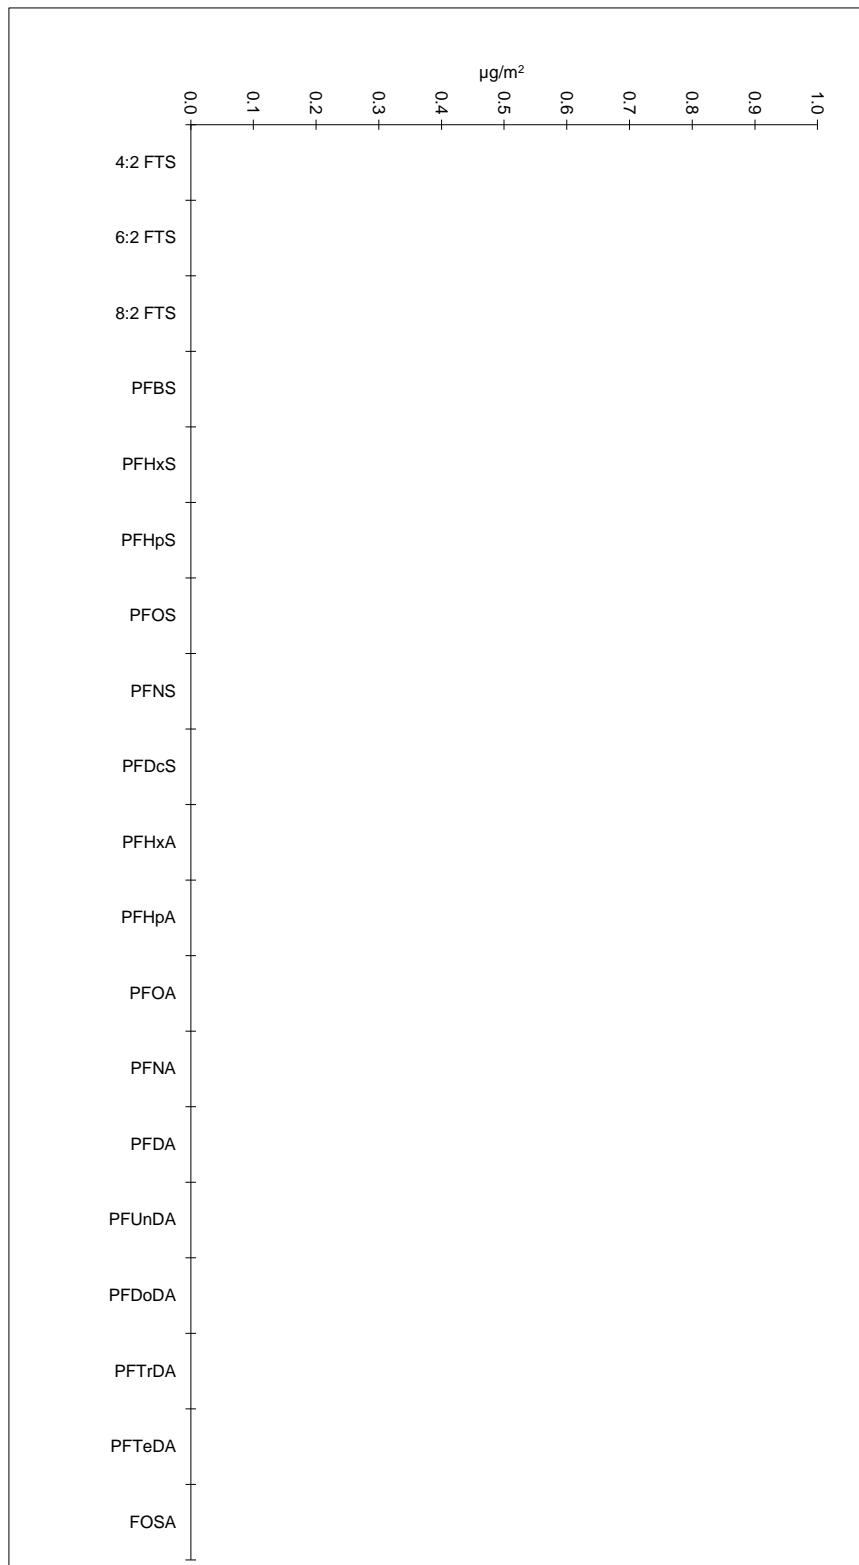

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 45
 Customer: Framtiden i våre hender
 Customers sample ID: Espressohouse sandwichpapir

Type of sample: Matemballasje
 Sample amount (g): 0.36
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	<0.94
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.56
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.7
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 45

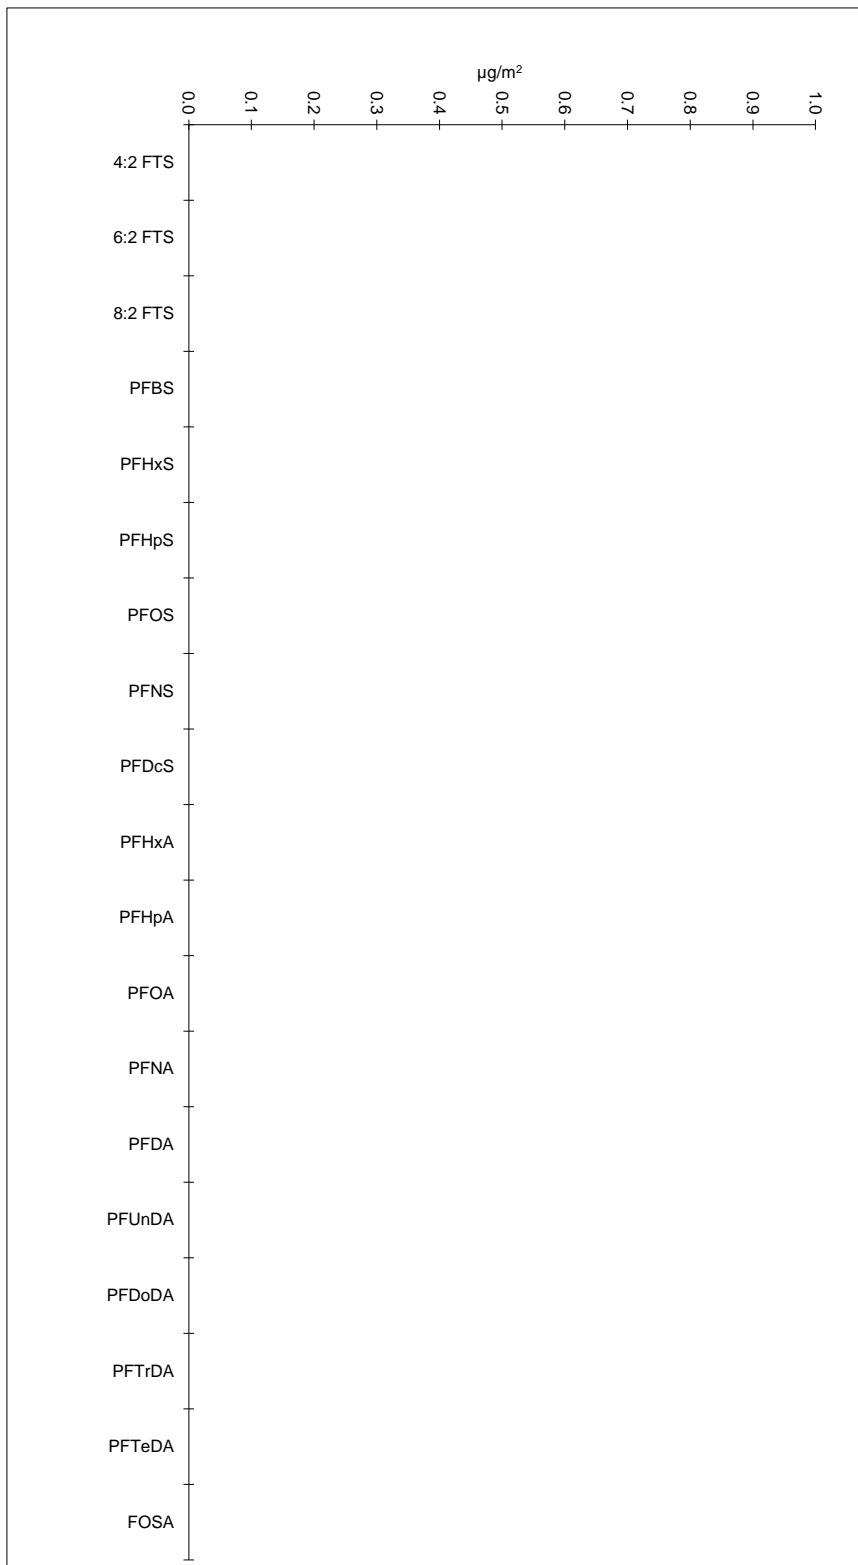

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 46
 Customer: Framtiden i våre hender
 Customers sample ID: 7/11 pizzapapp

Type of sample: Matemballasje
 Sample amount (g): 0.52
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	<0.97
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.56
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.7
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 46

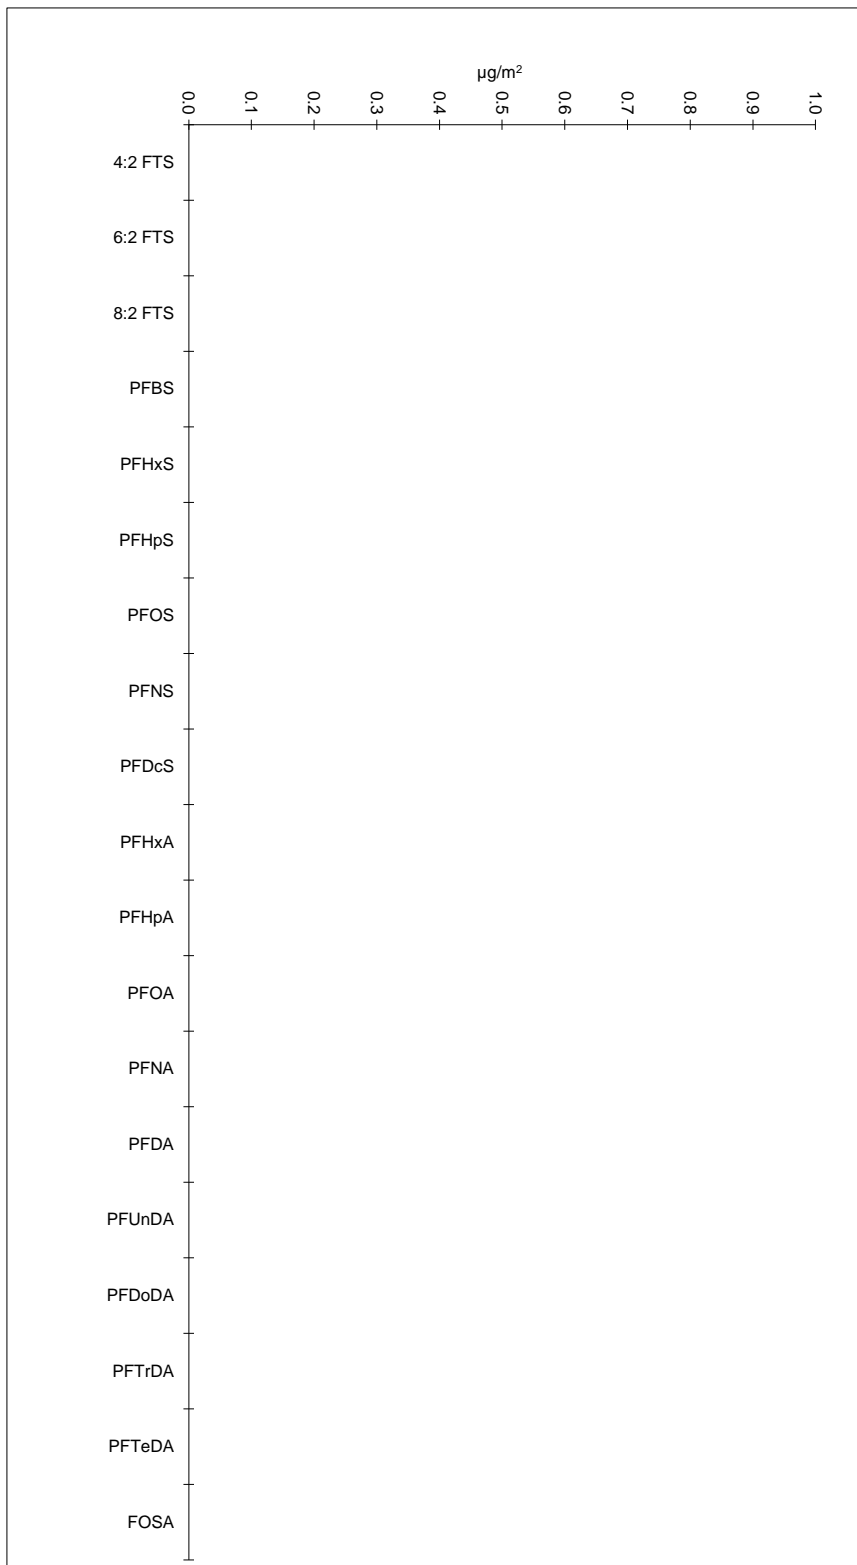

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 47
 Customer: Framtiden i våre hender
 Customers sample ID: Big bite sandwichpapir

Type of sample: Matemballasje
 Sample amount (g): 0.29
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	<0.88
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.58
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.53
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 47

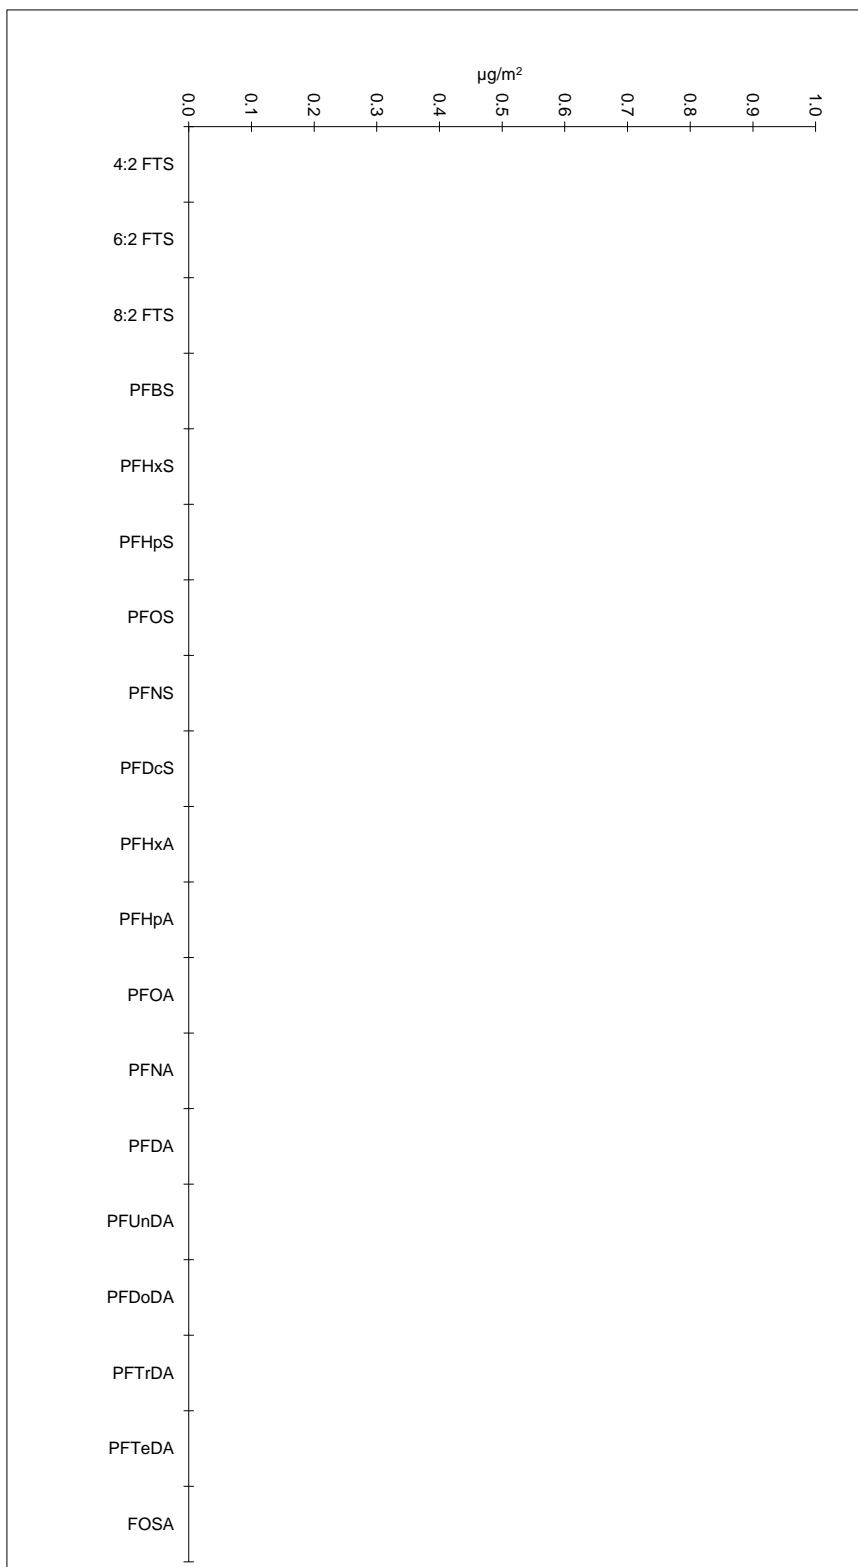

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 48
 Customer: Framtiden i våre hender
 Customers sample ID: Mc Donalds Hamburgereske

Type of sample: Matemballasje
 Sample amount (g): 1.00
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	249
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.56
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.52
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 48

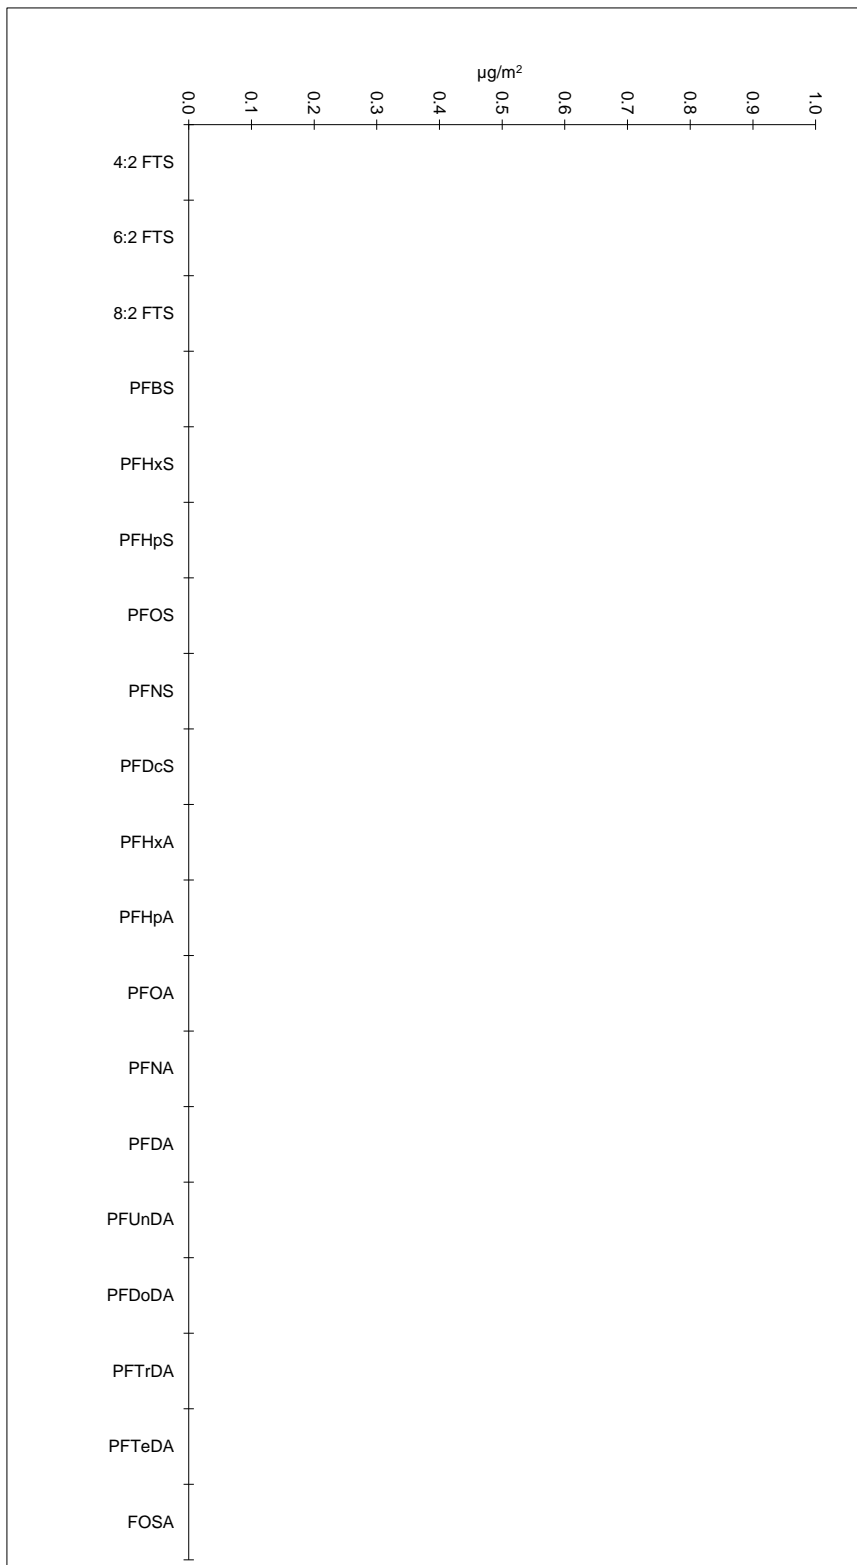

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 49
 Customer: Framtiden i våre hender
 Customers sample ID: Deli De Luka Muffinspapir

Type of sample: Matemballasje
 Sample amount (g): 2.83
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	<0.92
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.67
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.7
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 49

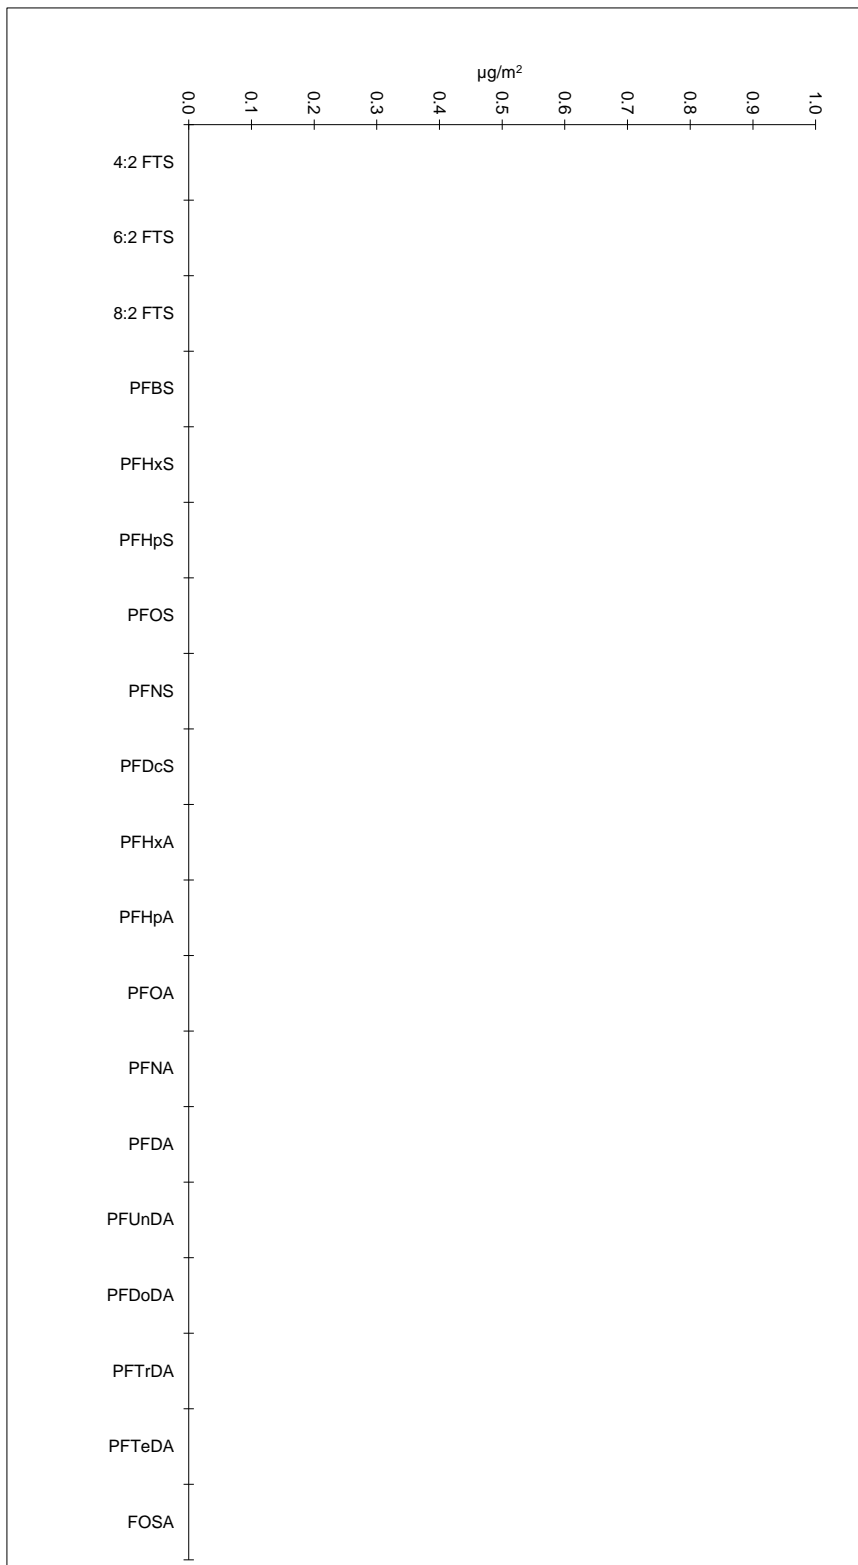

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 51
 Customer: Framtiden i våre hender
 Customers sample ID: Dolly Dimples pizzapapir

Type of sample: Matemballasje
 Sample amount (g): 2.74
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<0.1
	6:2 Fluorotelomer alcohol	6:2 FTOH	<0.83
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.57
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.41
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 51

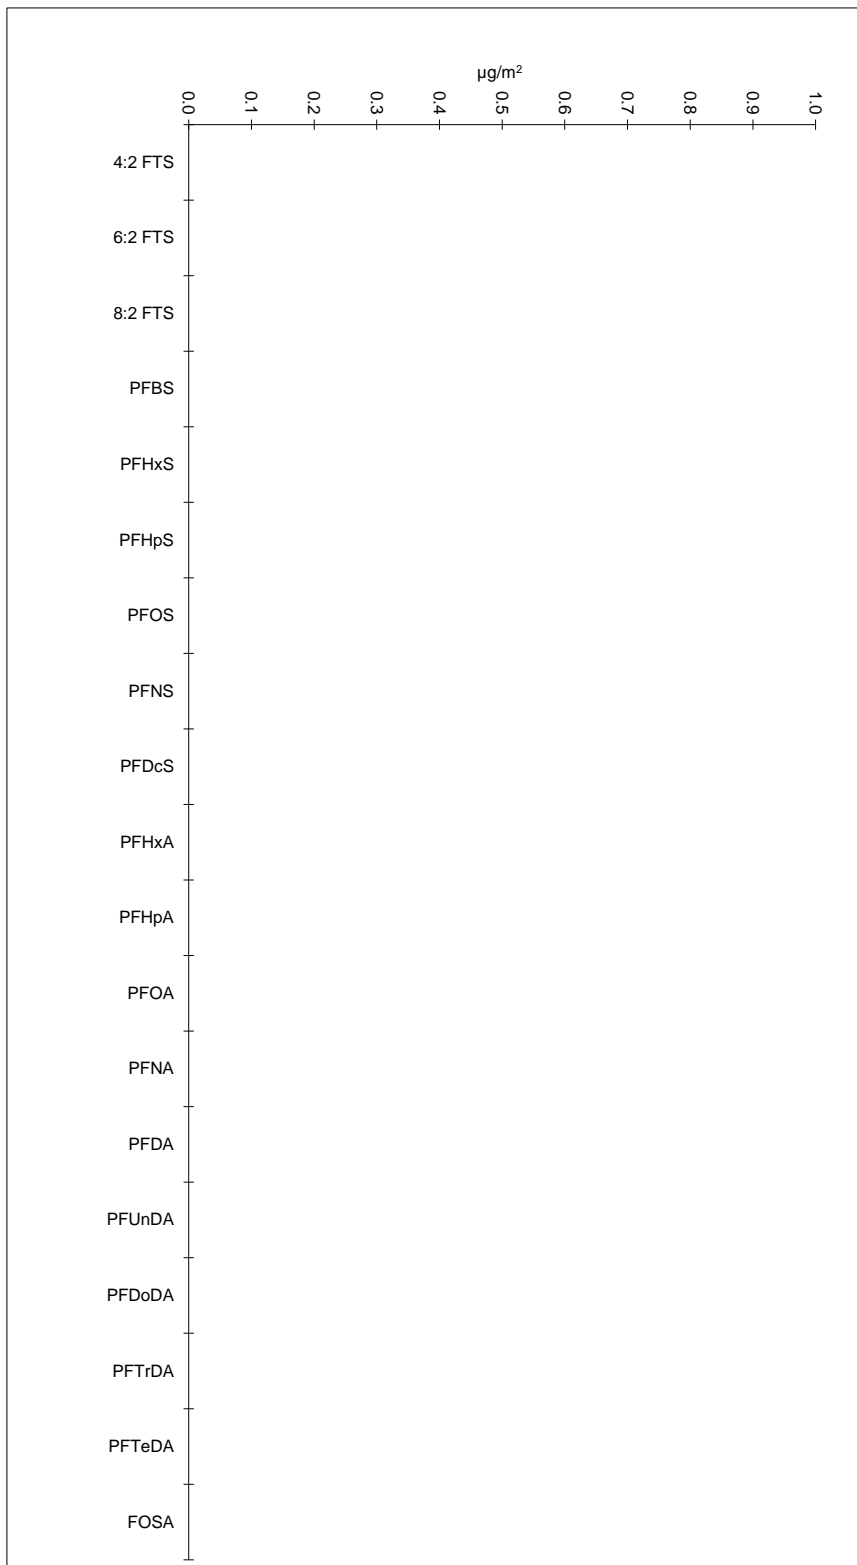

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 52
 Customer: Framtiden i våre hender
 Customers sample ID: Subway sandwich 1 papir

Type of sample: Matemballasje
 Sample amount (g): 0.30
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	<0.77
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.52
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.59
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 52

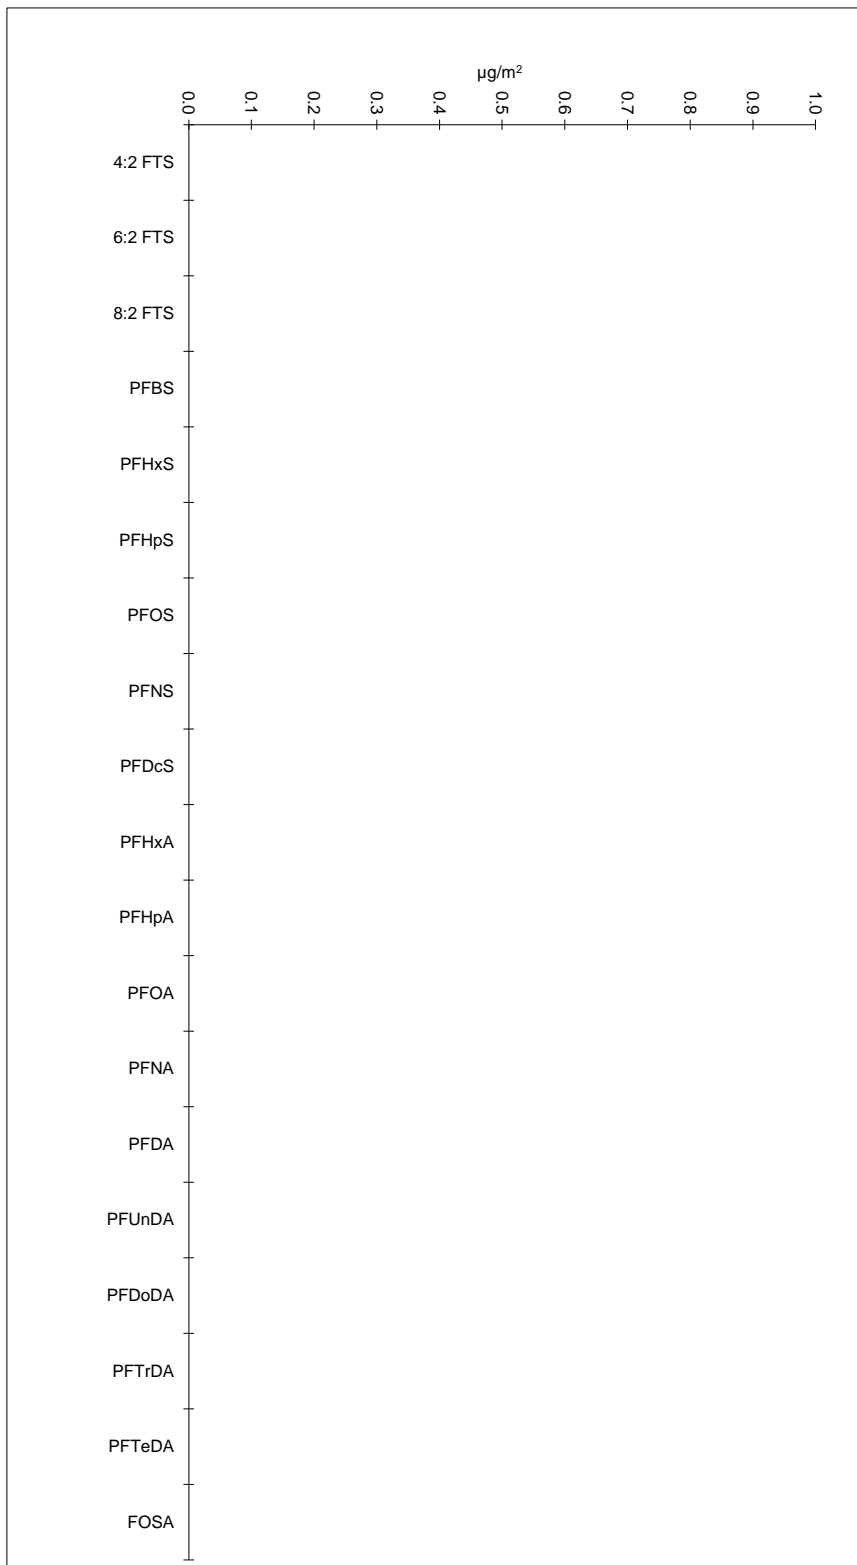

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 53
 Customer: Framtiden i våre hender
 Customers sample ID: Burger king pommes frites pose

Type of sample: Matemballasje
 Sample amount (g): 1.88
 Sample area (cm²): 100
 Measuring unit: µg/m²


Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	37.5
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.51
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.7
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 53

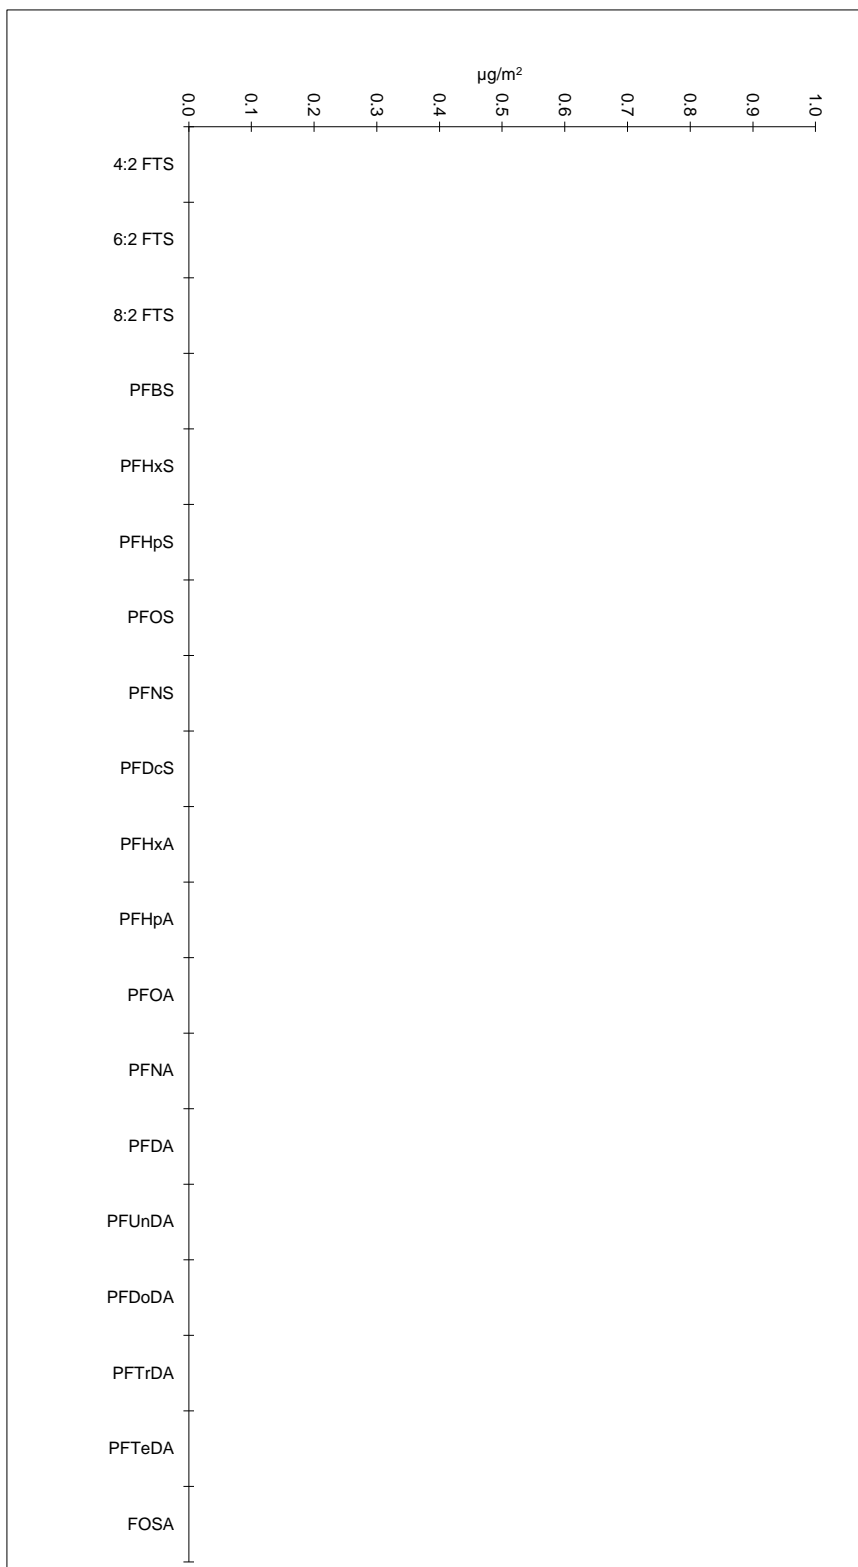

PFASs analysis results

Appendix to report: O-117039/43-54
 NILU sample number: 54
 Customer: Framtiden i våre hender
 Customers sample ID: Narvesen pizzaplate

Type of sample: Matemballasje
 Sample amount (g): 0.63
 Sample area (cm²): 100
 Measuring unit: µg/m²

Compound	Full name	Abbreviation	Concentration µg/m ²
	4:2 Fluorotelomer sulfonic acid	4:2 FTS	<0.02
	6:2 Fluorotelomer sulfonic acid	6:2 FTS	<0.01
	8:2 Fluorotelomer sulfonic acid	8:2 FTS	<0.01
	<i>Sum-FTS and FTCAs</i>		0
	Perfluorobutane sulfonate	PFBS	<0.01
	Perfluorohexane sulfonate	PFHxS	<0.01
	Perfluoroheptane sulfonate	PFHpS	<0.01
	Perfluorooctane sulfonate	PFOS	<0.01
	Perfluorononane sulfonate	PFNS	<0.02
	Perfluorodecane sulfonate	PFDCS	<0.02
	<i>Sum-PFSA</i>		0.00
	Perfluorohexanoate	PFHxA	<0.02
	Perfluoroheptanoate	PFHpA	<0.01
	Perfluorooctanoate	PFOA	<0.01
	Perfluorononanoate	PFNA	<0.01
	Perfluorodecanoate	PFDA	<0.01
	Perfluoroundecanoate	PFUnDA	<0.01
	Perfluorododecanoate	PFDoDA	<0.01
	Perfluorotridecanoate	PFTrDA	<0.02
	Perfluorotetradecanoate	PFTeDA	<0.02
	<i>Sum-PFCA</i>		0.0
	Perfluorooctane sulfonamide	FOSA	<0.01
	4:2 Fluorotelomer alcohol	4:2 FTOH	<1
	6:2 Fluorotelomer alcohol	6:2 FTOH	1.84
	8:2 Fluorotelomer alcohol	8:2 FTOH	<0.57
	10:2 Fluorotelomer alcohol	10:2 FTOH	<0.7
	Methylperfluorooctane sulfonamide	N-MeFOSA	n.a.
	Ethylperfluorooctane sulfonamide	N-EtFOSA	n.a.
	Methylperfluorooctane sulfonamidoethanol	N-MeFOSE	n.a.
	Ethylperfluorooctane sulfonamidoethanol	N-EtFOSE	n.a.

n.a: not analysed

<: Lower than indicated method detection limit (signal:noise 3:1)

PFAS analysis results

Appendix to report: O-117039/43-54
NILU sample number: 54

